

Report No. : ECR2331020

page : 1 of 3



Report Date : 2023/8/14

Applicant : Tamsui MacKay Memorial Hospital Clinical Trial Pharmacy

Equipment Name : IP Cabinet Side(1F, Mackay Building_ Clinical Trial Pharmacy)

Customer Address : Clinical Trial Pharmacy, 1F Mackay Building, No.47, Minquan Rd., Tamsui District, New Taipei City 251404(1F, Mackay Building_ Clinical Trial Pharmacy)


Measurement Date : 2023/8/8

Measurement Item : Temperature & Humidity Measurement

Measurement Code : Operate according to customer's requirement

Measurement Results : See Pages

This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com.tw/Terms-and-Conditions> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com.tw/Terms-and-Conditions>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested.

						Report No. : ECR2331020	page : 2 of 3
Applicant	Tamsui MacKay Memorial Hospital Clinical Trial Pharmacy						
Equipment	IP Cabinet Side(1F, Mackay Building_ Clinical Trial Pharmacy)						
Manufacturer	ADTEK	Model	HTO-1-N-R-L-N-D24-4	Serial No.	5101-20221213009-00001		
Procedure used	operate according to customer's requirement	Received Date	2023/8/8	Measurement Date	2023/8/8		
Examiner	Luke Tsai	Temperature(°C)	(22 ~ 22) °C	Relative Humidity(%)	(62 ~ 53) %		
Customer Address	Clinical Trial Pharmacy, 1F Mackay Building, No.47, Minquan Rd., Tamsui District, New Taipei City 251404(1F, Mackay Building_ Clinical Trial Pharmacy)						

SGS Standards

Equipment	Manufacturer	Model	Calibration Date
Thermo Hygrometer + Sensor	DELTA OHM	HD2301.0/HP474AC	2023/7/5
Serial Number	Traceability	Report No	Due Date
08034286+08035913	SGS(TAF 0143)	ECR2324881	2024/7/4

- ★ Reproduced report in partial is not effective without approval by SGS.
- ★ The results of the inspection are only effective for the samples inspected.
- ★ The sketch or photograph As refer to following pages.
- ★ Please refer to following pages to see the inspection result.

Luke Tsai

Examiner

Ken Ting

Approval Signatory

This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com.tw/Terms-and-Conditions> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com.tw/Terms-and-Conditions>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested.


台灣檢驗科技

1. Measurement purpose

SGS CM Lab is according to customer's request to measure temperature & humidity.
The results based on the measurement data need to ensure that environment within the allowable temperature and humidity range.

2. Measurement locations

Applicable to the location RCH溫濕度感測器 IP Cabinet Side.

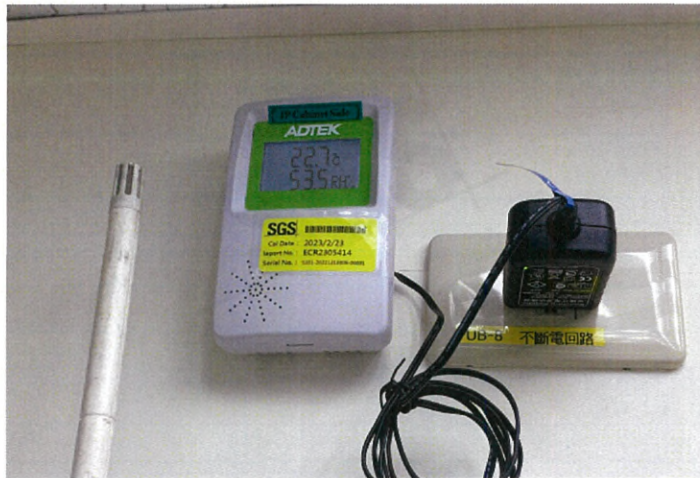

3. Temperature & Humidity Measurement Results :

Number of Measurements	Measured Value		Actual Value		Deviation	
	Temperature (°C)	Humidity (%)	Temperature (°C)	Humidity (%)	Temperature (°C)	Humidity (%)
1	22.8	53.5	21.9	52.9	0.9	0.6
2	22.7	53.5	21.8	53.0	0.9	0.5
3	22.8	53.4	21.9	53.0	0.9	0.4
4	22.7	53.4	21.8	52.9	0.9	0.5
5	22.7	53.3	21.8	52.9	0.9	0.4
Average	22.7	53.4	21.8	52.9	0.9	0.5

Deviation = Measured Value - Actual Value

---THE END---